


ThinPrep® Body Fluids Specimen Collection

Quick reference guide

WARNING: Do not process a cerebrospinal fluid (CSF) specimens or other sample type that is suspected of possessing prion infectivity (PrPsc) derived from a person with a TSE, such as Creutzfeldt-Jakob disease, on a ThinPrep® processor. A TSE contaminated processor cannot be effectively decontaminated and therefore must be properly disposed of in order to avoid potential harm to users of the processor or service personnel.




1. Collection.

Collect body fluids fresh.


Note:

- Fluids collected in ThinPrep® CytoLyt® solution require a CytoLyt solution wash prior to instrument processing.
- For extremely bloody fluids (i.e., pericardial), start with only 10 mL of fresh fluid.
- Urine may be collected into ThinPrep® PreservCyt® solution. A 2:1 urine-to-PreservCyt ratio is required. The ThinPrep® UroCyt® urine collection kit with PreservCyt® solution is recommended.



5. Evaluate cell pellet appearance.

Refer to Procedure B on opposite side of page.



2. Concentrate by centrifugation.

Centrifuge at 600g for 10 minutes or 1200g for 5 minutes.




6. Add an appropriate amount of specimen (dependent on the size of the cell pellet) to the PreservCyt solution vial.

Refer to Procedure C on opposite side of page.



3. Pour off supernatant and resuspend cell pellet.

Refer to Procedure A on opposite side of page.




7. Allow to stand in PreservCyt solution for 15 minutes.



4. Add CytoLyt solution wash.

- Add 30 mL of CytoLyt solution.
- Centrifuge.
- Pour off supernatant.
- Resuspend cell pellet.



8. Run on either the ThinPrep® 2000 processor using Sequence 2 (FLU/FNA), ThinPrep® Genesis™ processor, ThinPrep® 5000 processor or ThinPrep® 5000 processor with AutoLoader using Sequence Non-Gyn.

Fix, stain, and evaluate.

Instructions for body fluids

Procedure A




Pour off supernatant and vortex to resuspend cell pellet.

Pour off the supernatant completely to effectively concentrate the sample. To do this, invert the centrifuge tube 180 degrees in one smooth movement, pour off all the supernatant, and then return the tube to its original position as shown in Figure 1. Observe the cell pellet during inversion to avoid accidental loss of cellular material.

Caution: Failure to completely pour off the supernatant may produce a sparse sample and an unsatisfactory slide due to dilution of the cell pellet.


Resuspension can be done on a vortexor or may be achieved by syringing the pellet back and forth with a plastic pipette.

Figure 1.
Pouring off supernatant

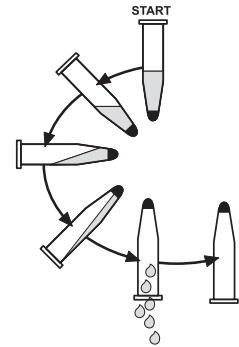

Procedure B

Evaluate cell pellet appearance.






Appearance of cell pellet	Procedure
Cell pellet is white, pale pink, tan or not visible.	Add specimen to PreservCyt solution vial. See Procedure C.
Cell pellet is distinctly red or brown indicating the presence of blood.	CytoLyt solution wash. - Add 30 mL of CytoLyt solution. - Concentrate by centrifugation. - Pour off supernatant and vortex to resuspend cell pellet.
Cell pellet is mucoid (not in liquid form). To test for liquid form, draw a small amount of the sample into a pipette and deliver drops back into the tube. If the drops appear stringy or gelatinous, then the mucus must be further liquefied.	CytoLyt solution wash. - Add 30 mL of CytoLyt solution. - Mechanical agitation. - Concentrate by centrifugation. - Pour off supernatant and vortex to resuspend cell pellet.

Procedure C

Add specimen to PreservCyt solution vial.

Determine the cell pellet size and refer to the table below:



Size of cell pellet	Procedure
 Pellet is clearly visible and the pellet volume is less than 1 mL.	Place the centrifuge tube in a vortexor to resuspend the cells in the residual liquid or mix the pellet by syringing it manually with a pipette. Transfer 2 drops of the pellet to a fresh PreservCyt solution vial.
 Pellet is not visible or is scant.	Add the contents of a fresh PreservCyt solution vial (20 mL) into the tube. Vortex briefly to mix the solution and pour the entire sample back into the PreservCyt solution vial.
 Pellet volume is greater than 1 mL.	Add 1 mL of CytoLyt solution into the tube. Vortex briefly to resuspend the pellet. Transfer 1 drop of the specimen to a fresh PreservCyt solution vial.

See your ThinPrep® Processor Operator's Manual for more information.

For technical support call 800-442-9892 - Option 1.

References: 1. MAN-02585-001 ThinPrep 2000 Processor Operator's Manual. Section 2: ThinPrep 2000 For Non-Gynecologic Use; Ch. 1; Section E-3 pg. 1.20-1.21
2. MAN-05394-001 ThinPrep Genesis Processor Operator's Manual. Ch. 5; Section E-3 pg. 5.20-5.21
3. MAN-06024-001 ThinPrep 5000 Processor Operator's Manual. Ch. 5; Section E pg. 5.17-5.18
4. MAN-06025-001 ThinPrep 5000 Processor with AutoLoader Operator's Manual. Ch. 5; Section C pg. 5.3-5.5

DS-09699-001 Rev. 002 © 2023 Hologic, Inc.. All rights reserved. Hologic, CytoLyt, PreservCyt, ThinPrep, UroCyt, Genesis and associated logos are trademarks and/or registered trademarks of Hologic, Inc. and/or its subsidiaries in the United States and/or other countries. All other trademarks are the property of their respective owners. This information is intended for medical professionals in the U.S. and other markets and is not intended as a product solicitation or promotion where such activities are prohibited. Because Hologic materials are distributed through websites, eBroadcasts and tradeshows, it is not always possible to control where such materials appear. For specific information on what products are available for sale in a particular country, please contact your Hologic representative or write to diagnostic.solutions@hologic.com.

ThinPrep®
NON-GYN